



Europäisches Patentamt  
European Patent Office  
Office européen des brevets



(11) EP 1 057 451 A2

(12)

## EUROPEAN PATENT APPLICATION

(43) Date of publication:  
06.12.2000 Bulletin 2000/49

(51) Int Cl.7: A61B 5/113, A61N 1/39

(21) Application number: 00850093.6

(22) Date of filing: 26.05.2000

(84) Designated Contracting States:  
AT BE CH CY DE DK ES FI FR GB GR IE IT LI LU  
MC NL PT SE  
Designated Extension States:  
AL LT LV MK RO SI

(72) Inventors:  
• Myklebust, Helge  
4025 Stavanger (NO)  
• Fossan, Helge  
4015 Stavanger (NO)

(30) Priority: 31.05.1999 NO 992611

(74) Representative: Hammar, Ernst  
Albhlms Patentbyrå Stockholm AB,  
Box 5581  
114 85 Stockholm (SE)

(71) Applicant: Laerdal Medical AS  
4001 Stavanger (NO)

(54) **System for measuring and using parameters during chest compression for cardio-pulmonary resuscitation or a simulation thereof**

(57) System for measuring parameters during chest compression in a life-saving situation or a practice situation, in which a pressure pad containing e.g. an accelerometer and a force activated switch (SW), as well as a calculation unit (B), is positioned on a patient's chest, alternatively on or inside a manikin's chest, in order to register parameters such as depression distance, duration or rate of depressions during chest compression, in a life-saving situation or a practice situation.

The accelerometer may be installed on a printed circuit board arranged at right angles on the pressure pad that is to be positioned on a patient's or manikin's chest, or the printed circuit board may be placed inside the manikin's chest.

The pressure pad may be provided with markings

on the top surface for guidance regarding placement on a patient's or a manikin's chest.

The pressure pad or a unit connected to the pressure pad contains a calculation unit (B) for calculation of the compression depth dependence on the acceleration values.

The pressure pad may contain a separate information unit, for instance consisting of light-emitting diodes (LEDs), or the sensor unit may have an outlet that can be connected to a display unit such as a screen, for display of a curve showing compression depth(Sn) versus time, possibly together with other signals such as the ECG curve and inflation.

Said outlet may in addition form an interface to a computer and/or a modem.

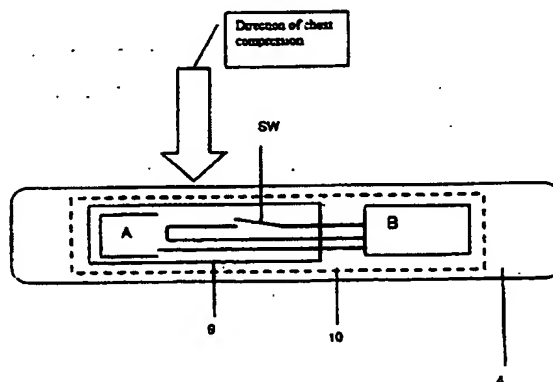


Fig. 6

EP 1 057 451 A2

## Description

[0001] The present invention regards a system for measuring and using parameters during chest compression in a life-saving situation or a practice situation, as stated in the introduction to Claim 1, and also an application as stated in Claim 11. Further characteristics of the invention will be seen from the remaining, dependent claims. The system may be connected to devices for performance feedback, in order to increase quality and efficiency.

[0002] Chest compression is a part of cardio-pulmonary resuscitation (CPR). CPR is described as life-saving first aid, and is part of the treatment given in case of sudden cardiac death. The compression depth is an important parameter during chest compression, which distance is given in centimetres in the CPR guidelines. Up until now, it has not been possible to measure this quantity in a sensible manner in connection with chest compressions on humans. In practice situations involving manikins on the other hand, it is common practice to measure and feed this information back to the lifesaver. Through practising chest compression on a manikin, the lifesaver should be capable of repeating the same movement pattern on humans. Two facts make this difficult: First of all, studies show that a lot of people's ability to repeat this movement pattern is poor already immediately after being trained. Likewise, studies show that the ability to repeat the movement pattern is lessened further over time. Secondly, people who are to be given chest compressions will offer different degrees of resistance to the depression, as the human anatomy varies. As such, an assessment of the compression depth cannot be made on the basis of the force applied. The quality of the chest compression will be completely dependent on the ability of the rescuer to transfer what he or she has learnt in the practice situation, and his or her ability to judge the depth and rate of compressions.

[0003] Studies in several countries have looked at the connection between the quality of cardiopulmonary resuscitation (CPR) and survival. These have indicated that the survival rate increases by a factor of 3-4 in the case of high quality CPR.

[0004] The object of the present invention is therefore to make it possible to improve the quality of chest compressions, such that a larger number of patients survive.

[0005] The above is provided through a device of the type mentioned initially, the characteristics of which can be seen from Claim 1. Further characteristics of the invention can be seen from the remaining, dependent claims.

[0006] Feedback may be in the form of a visual representation or in the form of corrective and instructive voice messages to the user; or the feedback may be forwarded to an emergency centre that can interpret the situation and guide the user during the life-saving. The data collected, or the feedback, may also be stored in order to provide documentation of the treatment administered to the patient, and may if necessary be compared with the CPR guidelines, for the purpose of improving the training system if possible.

[0007] The device according to the invention may be integrated in a defibrillator (AED) or be part of a device that measures and feeds back information regarding both compression and ventilation, or be a stand-alone device that only performs compression measurements and provides feedback, or it may form that part of the manikin sensor system which measures and registers chest compression.

[0008] In the following, the invention will be described in greater detail with reference to the drawings, in which:

Fig. 1 schematically shows a manikin with a compression unit for implementation of the invention.

Fig. 2 shows a curve diagram of measurement values relative to chest displacement.

Fig. 3 schematically shows a pressure pad containing the compression unit connected to the defibrillator patient cable.

Fig. 4 schematically shows an embodiment in which the pressure pad containing the compression unit is a stand-alone unit.

Fig. 5 shows a second embodiment of the pressure pad containing the compression unit.

Fig. 6 shows the principles of construction for the pressure pad

Fig. 7 shows the principal arrangement using two accelerometers in order to reduce measurement errors for chest compression performed during transport

[0009] The device may consist of a pad 4 that is connected to the patient's chest, the pad 4 having a supply cable with a terminal 1 for connection to electrodes 2. The top of the pad may be provided with instructions for placement of the pad in relation to the patient's nipples. The pad 4 provides a marker indicating where the lifesaver should put his hands in order to administer compressions, and also contains a sensor unit 9 for measuring depression, and possibly an additional sensor for the applied force. The sensor unit 9 consists of an accelerometer A and a force activated switch SW, and is connected to a calculation unit B in the form of for instance an electronic circuit. The force activated switch SW can be in the form of a membrane switch, and is arranged in the sensor unit 9 so that the applied vertical force is activating it. Together, the sensor unit 9 and the calculation unit B form the compression unit 10, see also Figure 6.

[0010] Accelerometer A may be of the type ADXL202 marketed by "Analog Devices", and may be provided on a

printed circuit board arranged at right angles to the surface of the pad on which the lifesaver puts his hands. Upon depression of the pad, the printed circuit board with the accelerometer will move, and the sensor will deliver an acceleration signal.

[0011] The depression is obtained by integrating the acceleration twice. In order to produce this result only, the initial parameters are set to zero at time  $t=0$ .

The two integrations yield:

$$\begin{aligned} (1) \int (\text{acceleration}) dt &= \text{Velocity} + V_0 & \text{Velocity at time } t=0: V_0 &= 0 \\ (2) \int (\text{acceleration}) dt &= \text{Distance} + D_0 & \text{Displacement at time } t=0: D_0 &= 0 \end{aligned}$$

In practice, this means that an integration circuit must be given the message to start the integration just as the depression commences. This will minimise integration errors caused by other factors.

[0012] The force activated switch SW being activated when the compression starts, or when the applied force measured exceeds a predetermined force can effect this.

[0013] The first solution of the integral gives the velocity, or speed, plus the initial velocity  $V_0$ , the initial velocity  $V_0$  being equal to zero when the integration commences upon activation of the switch, see also equation (1). The integration of the resulting velocity gives the displacement plus the initial position  $D_0$ . The initial position is equal to zero when the integration commences upon activation of the switch; see also equation (2).

[0014] The estimated displacement (distance)  $S_n$  is given by the following equation, which is deduced from the above integrals:

$$(3) \quad S_n \equiv S_{n-1} + \left( \frac{1}{2} \cdot a_n \cdot t_s^2 \right) + t_s^2 \cdot (a_0 + a_1 + a_2 + \dots a_{n-1})$$

in which  $n$  is the sample number,  $a_n$  is the acceleration, and  $t_s$  is the sample interval

[0015] Table I shows calculations performed by use of the rule in equation (3), where  $t_s$  is 1. Figure 2 shows the curve for the values in Table I.

Table I

Sample values	Acceleration [cm/s <sup>2</sup> ]	Calculation of depression $S_n$ [cm]
$A_0$	0	0
$a_1$	-2	-1
$a_2$	0	-3
$a_3$	2	-4
$a_4$	2	-3
$a_5$	0	-1
$a_6$	-2	0
$a_7$	0	0
$a_8$	0	0
$a_9$	0	0
$a_{10}$	0	0

[0016] If an accelerometer measuring the acceleration along two axes is used, the accelerometer may be oriented so as to let one measurement axis represent the vertical acceleration and the other the horizontal acceleration. Horizontal acceleration is undesirable, as it indicates that the applied chest compression is not vertical. In case of such an indication, the device will be able to give feedback to the user to the effect that the chest compression must be performed vertically.

[0017] This technique will be usable with other sensors, such as dynamometers, in order to obtain additional param-

eters for quality improvement.

[0018] Above, the invention has been described as used on a patient. However it will also be possible to use the invention for training purposes, by arranging the compression unit 10 unit either on or in a manikin, see Figure 1. The accelerometer can then be mounted on a plate in the manikin, which plate follows the chest compression in such a manner that the vertical acceleration indicates chest compression. Lung inflations can be measured by having the rising of the chest that is caused by the expansion of the manikin lungs act on an arm that rotates the plate on which the accelerometer is mounted, about an axis. Thereby the effect of gravity, g, on the accelerometer will cause the signal value to change. The compression unit 10 may also be used directly on the outside of the manikin, as if it were a patient. In this case, horizontal acceleration will indicate shaking in the manikin device. A force activated switch will also be provided here, in order to indicate the start of a chest compression, and the same calculations as mentioned above may be used to give an indication of the depression.

[0019] Using the unit according to the invention inside a manikin is advantageous when compared with previously used devices, as the new unit takes up little space compared with previously used units, which often consist of a toothed rack that co-operates with a sliding potentiometer in order to measure the displacement, and which becomes relatively large in size, thus leaving little space for other manikin equipment that is required in order to practice CPR and register all activity on the manikin.

[0020] The measured values can be transmitted to a separate calculation unit B that may be arranged in the pressure pad, as indicated in Fig. 4, or the measurement values are transmitted directly via separate supply leads 3 directly to a defibrillator 5 that employs its built-in CPU in order to perform the calculations, see also Figure 3. Said calculation unit B may for instance consist of a CPU unit and associated components for performing the calculations, and is technically considered to be prior art that anyone who is skilled in the art may implement. As such, it does not form part of the invention, and is not described in greater detail herein. When using a standard defibrillator 5 that is appropriate for this purpose, the information unit in this may be used to guide the lifesaver.

[0021] When using a stand-alone unit, this must be equipped with a separate CPU in order to perform the calculations, as well as a separate information unit. This information unit may simply consist of light-emitting diodes (LEDs) 6 as indicated in Figure 4. In the unit shown in Figure 4, the electronics and indicators are built into a pressure pad 4, which is provided with markings that show where on the patient the pressure pad should be placed and where the chest compression should be carried out. The light-emitting diodes may for instance indicate depression by one diode lighting up for each centimetre. When the depression exceeds 5 cm, the colour changes e.g. from green to red.

[0022] Figure 5 shows another possible embodiment of the invention, in which the pressure pad 4 has an outlet that can be connected to a display unit 7; for instance a screen, in order to provide feedback and possibly instructions. The estimated compression depth  $S_n$  being shown as indicated by the curve  $S_n$  in Figure 2. It may also show the inflations to the patient during the CPR. The inflation signal is produced in a known manner *per se*, by the display unit containing a measurement system that measures the impedance between the electrodes 2, and in which inflation causes a change in this impedance. The display unit 7 may also consist of a screen and a loudspeaker that provides feedback in the form of speech or sound signals, or a loudspeaker unit on its own. Instead of a separate display unit or in addition to the separate display unit, a computer may be connected for further processing of the data, or a modem or similar may be connected for transmission of data for instance to an emergency centre.

[0023] Figure 5 shows a connector 8 for connecting to the above-mentioned units or a defibrillator, which in addition to receiving the signals from the compression unit 4, also can receive signals (ECG) from the electrodes 2 or deliver electrical shocks via the electrodes 2.

[0024] Occasionally, CPR must be performed during transportation, like in an ambulance, in a boat or aeroplane. In these conditions, the accelerometer A will also be affected by the overall vertical movement of the vehicle, thus introducing an integration error on estimated chest compression depth  $S_n$ . Fig 7 shows the use of a second accelerometer A2, placed for instance within the defibrillator 5. This accelerometer is arranged to sense the vertical movement of the vehicle, and by subtracting the signal  $A2_n$  from the signal  $A_n$  from A using the calculation unit B, the integration error is significantly reduced.:

$$a_n = A_n - A2_n$$

#### Claims

1. System for measuring and using parameters when performing chest compression in a life-saving situation or a practice situation, wherein is included a calculation unit set to determine depression depth during compression by using signals from a sensor unit consisting of a force activated switch set to respond when the depression commences, thereby indicating the start of the movement, and an accelerometer set to follow the movement of the

chest.

2. System for measuring and using parameters when performing chest compression in a life-saving situation or a practice situation, wherein a calculation unit (B) is set to estimate compression depth as a function of the difference of the signals from a first accelerometer set to follow the movement of the chest, and a second accelerometer set to follow the movement of the patient.
3. System according to Claim 1 or 2, wherein the sensor unit is placed inside a pressure pad to be arranged on a patient's or manikin's chest.
4. System according to Claims 3, wherein the pressure pad is provided with markings on the top for guidance regarding placement on a patient's or manikin's chest.
5. System according to Claims 1 or 2, wherein the calculation unit is an electronic circuit arranged in the pressure pad.
6. System according to Claims 1 or 2, wherein the calculation unit determines the approximate depression depth  $S_n$  according to the equation

$$S_n = S_{n-1} + \left( \frac{1}{2} \cdot a_n \cdot t_i^2 \right) + t_i^2 \cdot (a_0 + a_1 + a_2 + \dots + a_{n-1})$$

in which  $n$  is the sample number,  $a_n$  is the acceleration, and  $t_i$  is the sample interval, the calculation being carried out for as long as the force activated switch is activated.

7. System according to Claims 3, wherein the pressure pad contains a separate feedback unit, for instance consisting of light emitting diodes, and/or an audio unit for providing feedback and possibly instructions in the form of speech.
8. System according to Claims 3, wherein the pressure pad includes an outlet that can be connected to a display unit, e.g. a screen, for display of a curve showing the depression depth versus time.
9. System according to Claims 3, wherein said outlet in the pressure pad forms an interface to a defibrillator, a computer and/or a modem.
10. System according to Claims 8, wherein the display unit includes a loudspeaker unit for providing feedback and any instructions in the form of speech.
11. Application of a system including a sensor unit, consisting of an accelerometer and a force activated switch connected to a calculation unit, that measures parameters such as depression depth and depression rate when chest compression is performed in a life-saving situation or a practice situation, in which the sensor unit and the calculation unit are arranged inside a pressure pad, together with means of providing feedback regarding performance, where the feedback may be visual and/or verbal or in the form of sound signals.
12. Application according to Claim 11 of a system that measures parameters when chest compression is performed in a life-saving situation or a practice situation, in which the sensor unit and the calculation unit are connected to a defibrillator, or alternatively the calculation unit forms an integral part of the defibrillator, and where the defibrillator includes means of providing feedback regarding the performance of the chest compression.
13. Application according to Claim 11 of a system that measures parameters when chest compression is performed in a practice situation, in which the sensor unit and the calculation unit are placed inside a manikin together with means for providing feedback regarding performance, where the feedback may be visual and/or verbal or in the form of sound signals.

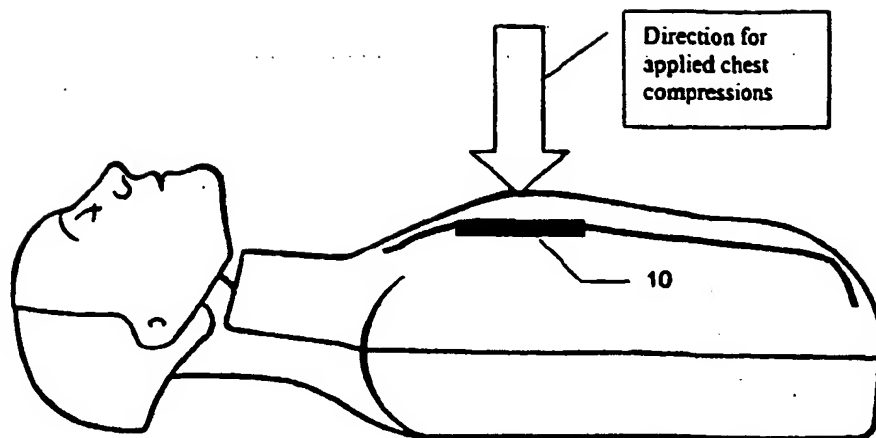


Fig. 1

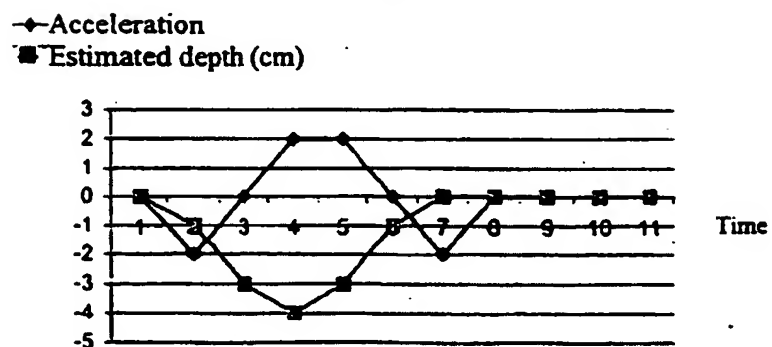


Fig. 2

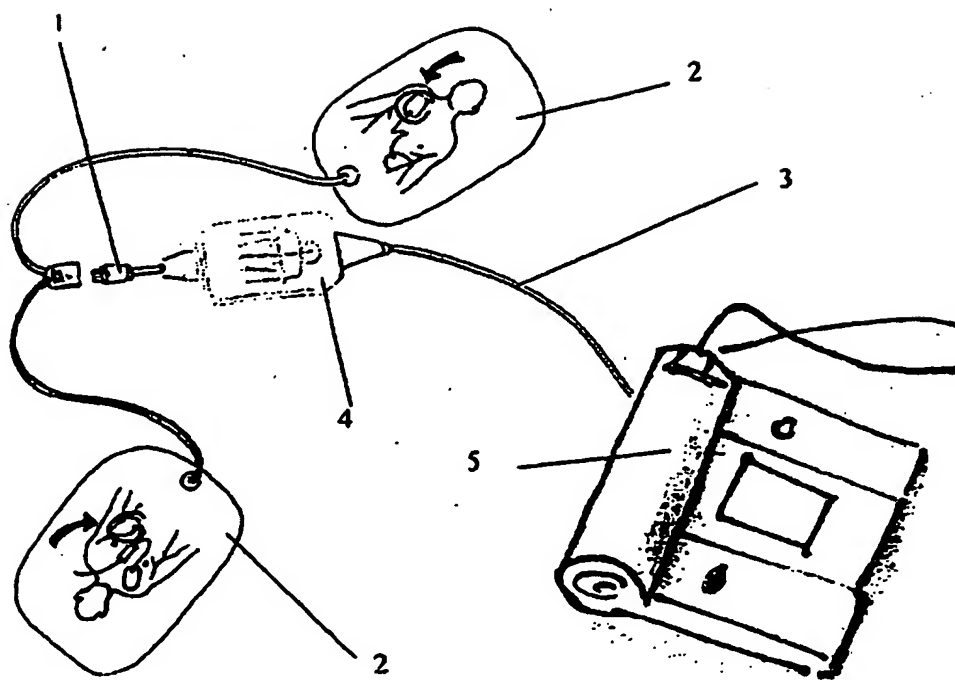


Fig. 3

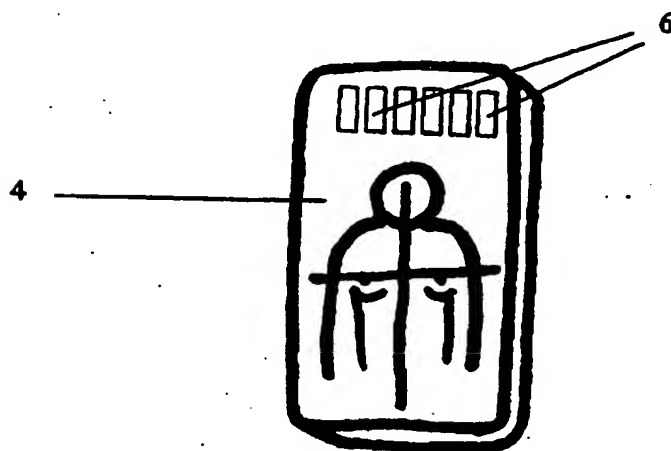


Fig. 4


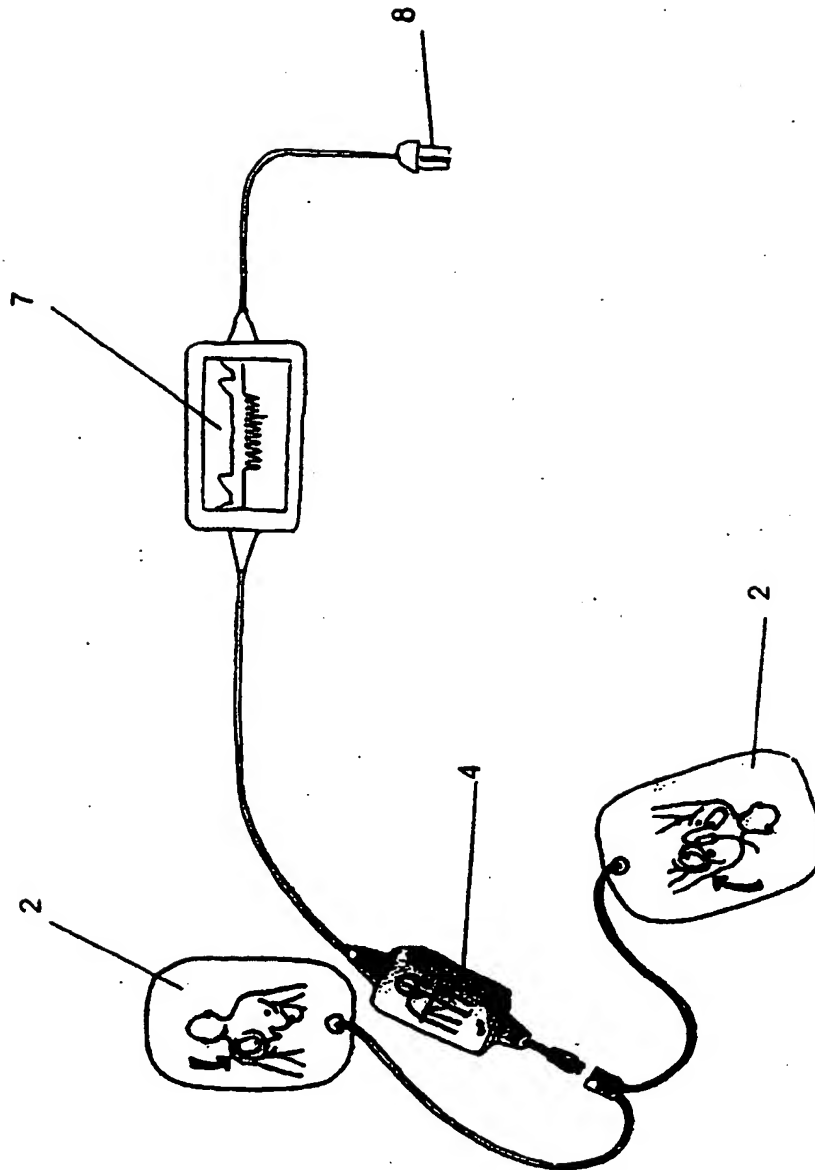


Fig. 5



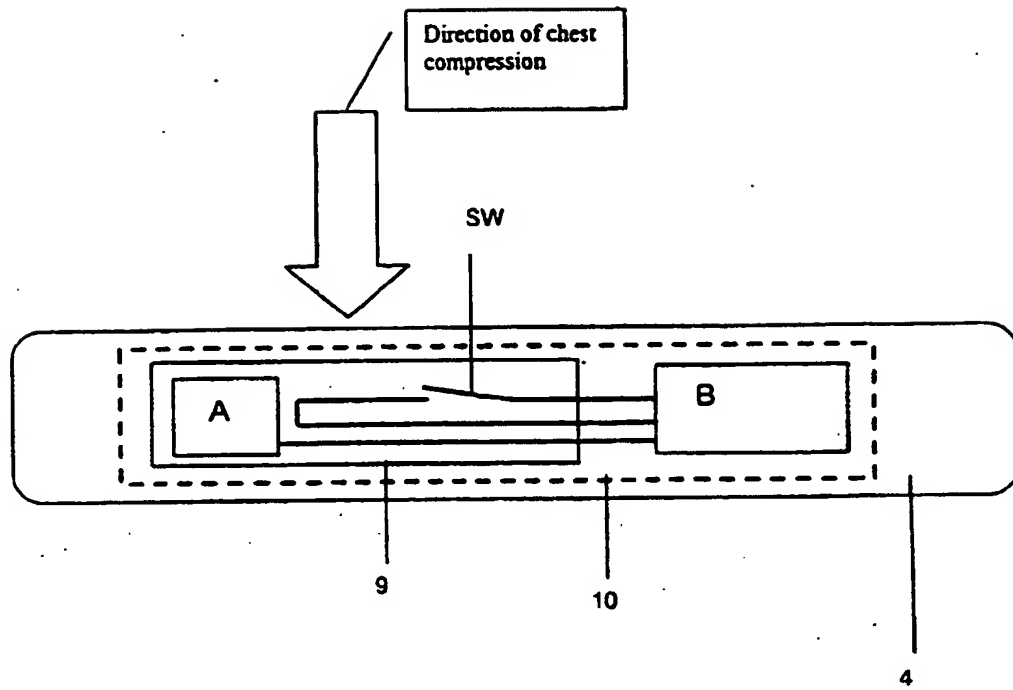

**Fig. 6**


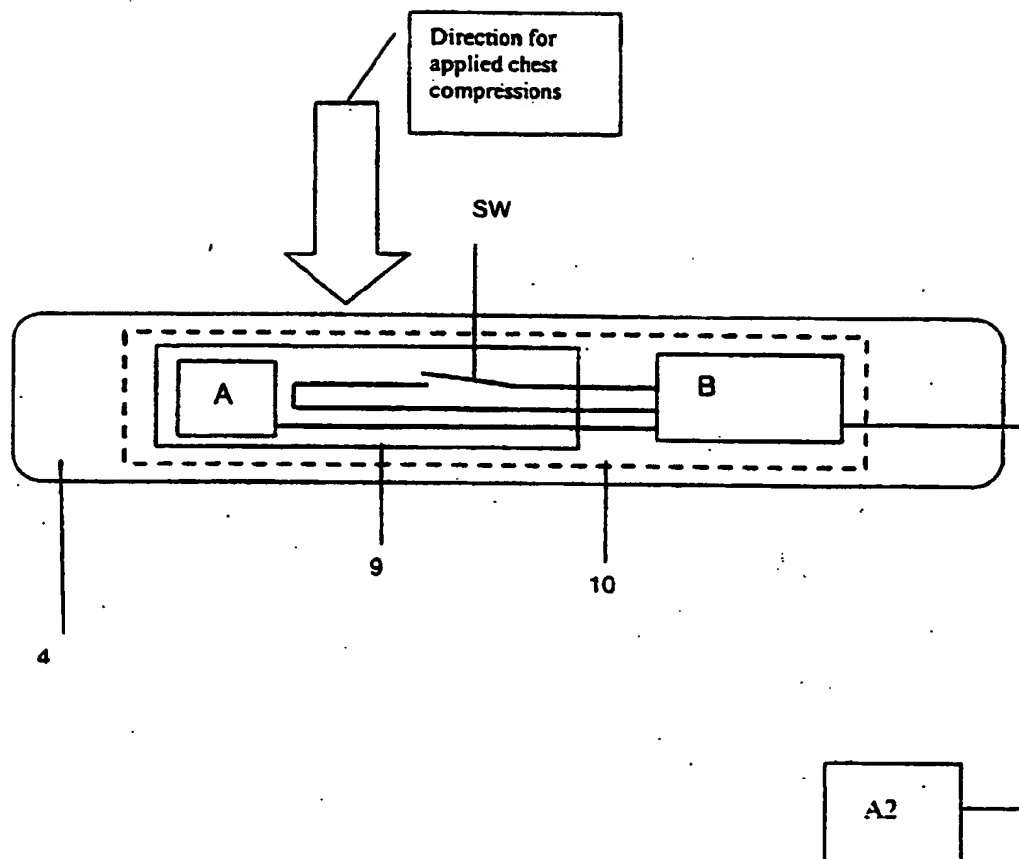


Fig. 7



Europäisches Patentamt  
European Patent Office  
Office européen des brevets



(11)

**EP 1 057 451 A3**

(12)

**EUROPEAN PATENT APPLICATION**

(88) Date of publication A3:  
24.03.2004 Bulletin 2004/13

(51) Int Cl.7: **A61H 31/00, G09B 23/28,  
A61B 5/113, A61B 5/103**

(43) Date of publication A2:  
06.12.2000 Bulletin 2000/49

(21) Application number: **00850093.6**

(22) Date of filing: **26.05.2000**

(84) Designated Contracting States:  
**AT BE CH CY DE DK ES FI FR GB GR IE IT LI LU  
MC NL PT SE**  
Designated Extension States:  
**AL LT LV MK RO SI**

(72) Inventors:  
• **Myklebust, Helge**  
4025 Stavanger (NO)  
• **Fossan, Helge**  
4015 Stavanger (NO)

(30) Priority: **31.05.1999 NO 992611**

(74) Representative: **Hammar, Ernst**  
**Albihns Stockholm AB,**  
**Box 5581**  
**114 85 Stockholm (SE)**

(71) Applicant: **Laerdal Medical AS**  
4001 Stavanger (NO)

(54) **System for measuring and using parameters during chest compression for cardio-pulmonary resuscitation or a simulation thereof**

(57) System for measuring parameters during chest compression in a life-saving situation or a practice situation, in which a pressure pad containing e.g. an accelerometer and a force activated switch (SW), as well as a calculation unit (B), is positioned on a patient's chest, alternatively on or inside a manikin's chest, in order to register parameters such as depression distance, duration or rate of depressions during chest compression, in a life-saving situation or a practice situation.


The accelerometer may be installed on a printed circuit board arranged at right angles on the pressure pad that is to be positioned on a patient's or manikin's chest, or the printed circuit board may be placed inside the manikin's chest.

The pressure pad may be provided with markings on the top surface for guidance regarding placement on a patient's or a manikin's chest.

The pressure pad or a unit connected to the pressure pad contains a calculation unit (B) for calculation of the compression depth in dependence on the acceleration values.

The pressure pad may contain a separate information unit, for instance consisting of light-emitting diodes (LEDs), or the sensor unit may have an outlet that can be connected to a display unit such as a screen, for display of a curve showing compression depth (Sn) versus time, possibly together with other signals such as the ECG curve and Inflation.

Said outlet may in addition form an interface to a computer and/or a modem.

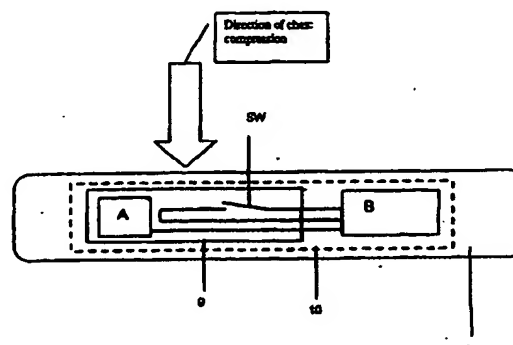

**Fig. 6**

**EP 1 057 451 A3**



European Patent  
Office

# EUROPEAN SEARCH REPORT

Application Number  
EP 00 85 0093

DOCUMENTS CONSIDERED TO BE RELEVANT			
Category	Citation of document with indication, where appropriate, of relevant passages	Relevant to claim	CLASSIFICATION OF THE APPLICATION (InCL.7)
P,A	WO 00 27464 A (EMERGENCY MEDICAL SYSTEMS INC) 18 May 2000 (2000-05-18) * the whole document *	1-3,5-8, 10,11,13	A61H31/00 G09B23/28 A61B5/113 A61B5/103
P,A	WO 99 63926 A (CPRX LLP) 16 December 1999 (1999-12-16) * the whole document *	1-4,6-12	
A	WO 99 25306 A (LAMISH AHARON ;CPR DEVICES LTD (IL); LASS YORAM (IL)) 27 May 1999 (1999-05-27) * page 12, line 34 - page 13, line 29 *	1-3, 6-11,13	
A	US 4 797 104 A (AAMODTH KJELL ET AL) 10 January 1989 (1989-01-10) * column 10, line 51-62 * * column 11, line 7-54 *	1,2,8,9, 11	
A	US 5 589 639 A (D ANTONIO NICHOLAS F ET AL) 31 December 1996 (1996-12-31) * column 4, line 20 - column 5, line 5 * * column 22, line 48 - column 24, line 57 *	1-3,5,7, 11,13	TECHNICAL FIELDS SEARCHED (InCL.7)
A	US 5 496 257 A (KELLY KENNETH B) 5 March 1996 (1996-03-05) * column 4, line 63 - column 7, line 2 * * column 10, line 14-41 *	1-5,7,8, 10,11,13	A61B G09B A61H A61N
A	US 4 828 501 A (INGENITO MICHAEL ET AL) 9 May 1989 (1989-05-09) * column 5, line 39-50 * * column 10, line 8-40 * * column 15, line 11 - column 16, line 5 *	1-3,5,7, 8,10,11, 13	
The present search report has been drawn up for all claims			
Place of search <b>THE HAGUE</b>		Date of completion of the search <b>30 January 2004</b>	Examiner <b>Smeyers, C</b>
<p><b>CATEGORY OF CITED DOCUMENTS</b></p> <p>X: particularly relevant if taken alone Y: particularly relevant if combined with another document of the same category A: technological background O: non-written disclosure P: intermediate document</p> <p>T: theory or principle underlying the invention E: earlier patent document, but published on, or after the filing date D: document cited in the application L: document cited for other reasons</p> <p>&amp;: member of the same patent family, corresponding document</p>			

EPO FORM 1503 (03.02 (04/00))

**ANNEX TO THE EUROPEAN SEARCH REPORT  
ON EUROPEAN PATENT APPLICATION NO.**

EP 00 85 0093

This annex lists the patent family members relating to the patent documents cited in the above-mentioned European search report. The members are as contained in the European Patent Office EOP file on  
The European Patent Office is in no way liable for these particulars which are merely given for the purpose of information.

30-01-2004

Patent document cited in search report		Publication date	Patent family member(s)	Publication date
WO 0027464	A	18-05-2000	US 6390996 B1	21-05-2002
			AU 2146500 A	29-05-2000
			EP 1128795 A2	05-09-2001
			JP 2002529157 T	10-09-2002
			US 2002165471 A1	07-11-2002
			WO 0027464 A2	18-05-2000
			US 2002193711 A1	19-12-2002
			US 2002055694 A1	09-05-2002
WO 9963926	A	16-12-1999	US 6234985 B1	22-05-2001
			US 6224562 B1	01-05-2001
			US 6312399 B1	06-11-2001
			AU 4435299 A	30-12-1999
			BR 9911093 A	20-02-2001
			CA 2334723 A1	16-12-1999
			EP 1098622 A2	16-05-2001
			JP 2002517283 T	18-06-2002
			WO 9963926 A2	16-12-1999
			US 2002188332 A1	12-12-2002
			US 6463327 B1	08-10-2002
WO 9925306	A	27-05-1999	AU 748550 B2	06-06-2002
			AU 1256599 A	07-06-1999
			BR 9814971 A	03-10-2000
			CA 2310618 A1	27-05-1999
			CN 1279599 T	10-01-2001
			EP 1033960 A1	13-09-2000
			WO 9925306 A1	27-05-1999
			JP 2001522707 T	20-11-2001
			NO 20002458 A	14-07-2000
			PL 340830 A1	26-02-2001
US 4797104	A	10-01-1989	OE 3638192 A1	19-05-1988
US 5589639	A	31-12-1996	US 5279163 A	18-01-1994
			US 4823619 A	25-04-1989
			US 4987783 A	29-01-1991
			AU 1729295 A	01-08-1995
			WO 9519556 A1	20-07-1995
			AT 144832 T	15-11-1996
			DE 68927397 D1	05-12-1996
			DE 68927397 T2	28-05-1997
			EP 0356482 A1	07-03-1990
			JP 3501886 T	25-04-1991
			WO 8907248 A1	10-08-1989

EPO FORM P/US

For more details about this annex : see Official Journal of the European Patent Office, No. 12/82

**ANNEX TO THE EUROPEAN SEARCH REPORT  
ON EUROPEAN PATENT APPLICATION NO.**

EP 00 85 0093

This annex lists the patent family members relating to the patent documents cited in the above-mentioned European search report. The members are as contained in the European Patent Office EDP file on  
The European Patent Office is in no way liable for these particulars which are merely given for the purpose of information.

30-01-2004

Patent document cited in search report		Publication date		Patent family member(s)	Publication date
US 5496257	A	05-03-1996	WO	9731608 A1	04-09-1997
			AU	4996996 A	16-09-1997
US 4828501	A	09-05-1989	US	4915635 A	10-04-1990
			US	4932879 A	12-06-1990

EPO FORM P0139

For more details about this annex : see Official Journal of the European Patent Office, No. 12/82

**This Page is Inserted by IFW Indexing and Scanning  
Operations and is not part of the Official Record**

**BEST AVAILABLE IMAGES**

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images include but are not limited to the items checked:

- ☐ **BLACK BORDERS**
- ☐ **IMAGE CUT OFF AT TOP, BOTTOM OR SIDES**
- ☐ **FADED TEXT OR DRAWING**
- ☐ **BLURRED OR ILLEGIBLE TEXT OR DRAWING**
- ☐ **SKEWED/SLANTED IMAGES**
- ☐ **COLOR OR BLACK AND WHITE PHOTOGRAPHS**
- ☐ **GRAY SCALE DOCUMENTS**
- ☒ **LINES OR MARKS ON ORIGINAL DOCUMENT**
- ☐ **REFERENCE(S) OR EXHIBIT(S) SUBMITTED ARE POOR QUALITY**
- ☐ **OTHER:** \_\_\_\_\_

**IMAGES ARE BEST AVAILABLE COPY.**

**As rescanning these documents will not correct the image problems checked, please do not report these problems to the IFW Image Problem Mailbox.**

**THIS PAGE BLANK (USPTO)**